



Triumphant Labs
4858 W Pico Blvd #1031 Los Angeles, CA 90019
hi@triumphantlabs.com
http://triumphantlabs.com


SAMPLE NAME: Bacteriostatic Water 10ml
SAMPLE CODE: VXP3-4VZC
RECEIVED DATE: 06/04/2026
PUBLISHED DATE: 06/09/2026



DECLARED IDENTITY	Bacteriostatic Water
MATRIX TYPE:	BACTERIOSTATIC WATER
SAMPLE NAME:	Bacteriostatic Water 10ml
SAMPLE SIZE:	10 mL
LOT CODE:	KEIBW2606

Sample	Test	Specification	Result	Status
Benzyl Alcohol Assay (HPLC)	HPLC	0.9% (v/v) ±10%	0.88 % (v/v)	CONFORMS
Fill volume / Net content	Gravimetric	—	10.00 mL	MEASURED
pH Determination	pH	4.5 – 7.0	6.21	CONFORMS

HPLC Chromatogram Report

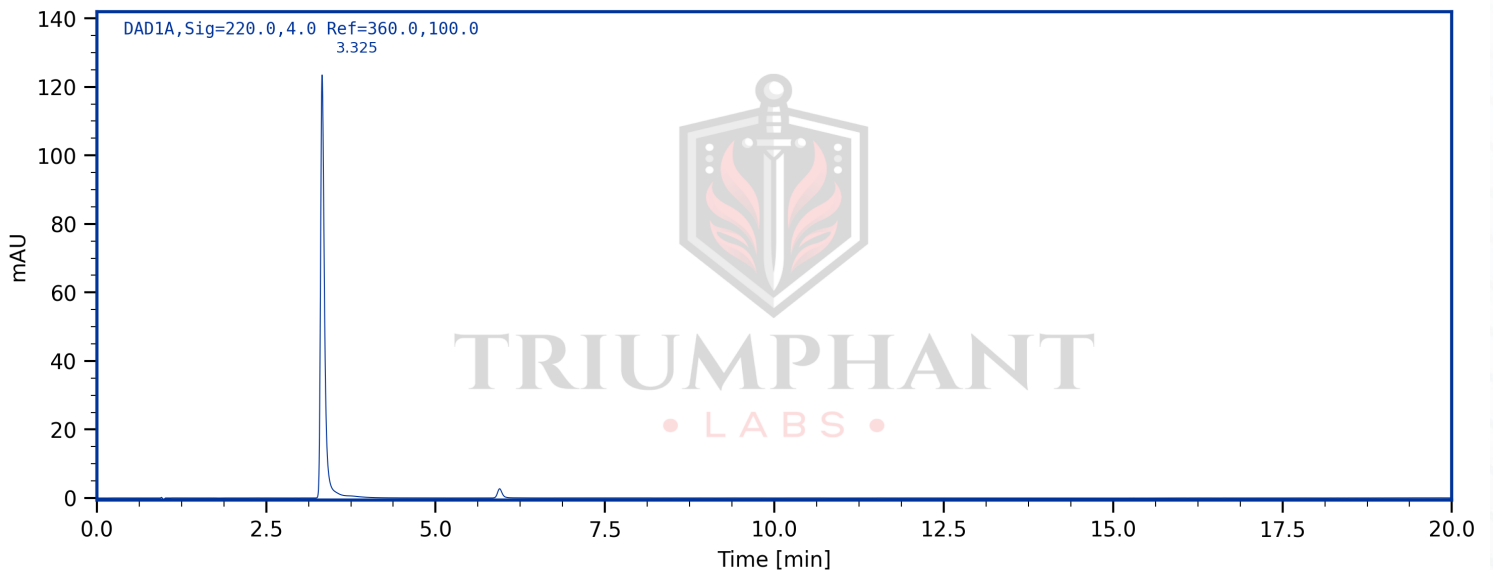

RESULTS REVIEWED BY:

Anthony Burke PhD
Lab Manager
06/09/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
06/09/2026

ACCUMARKLABS.COM
VXP3-4VZC
06/09/2026





Triumphant Labs
4858 W Pico Blvd #1031 Los Angeles, CA 90019
hi@triumphantlabs.com
http://triumphantlabs.com

SAMPLE NAME: Bacteriostatic Water 10ml
SAMPLE CODE: VXP3-4VZC
RECEIVED DATE: 06/04/2026
PUBLISHED DATE: 06/09/2026

Sample	Test	Specification	Result	Status
Benzyl Alcohol Assay (HPLC)	Endotoxin (LAL)	< 5.0 EU/mL	Pass	CONFORMS
Benzyl Alcohol Assay (HPLC)	Rapid Sterility Screening (PCR)	Not Detected	Pass	CONFORMS

RESULTS CERTIFIED BY:

RESULTS CERTIFIED BY:


Anthony Burke PhD
Lab Manager
06/09/2026


Dr. Levi Fried MD
Lab Director
06/09/2026

ACCUMARKLABS.COM
VXP3-4VZC
06/09/2026

